


Verpackungsanweisung für Rücklieferungen von Temperaturfühlerpaaren an JUMO

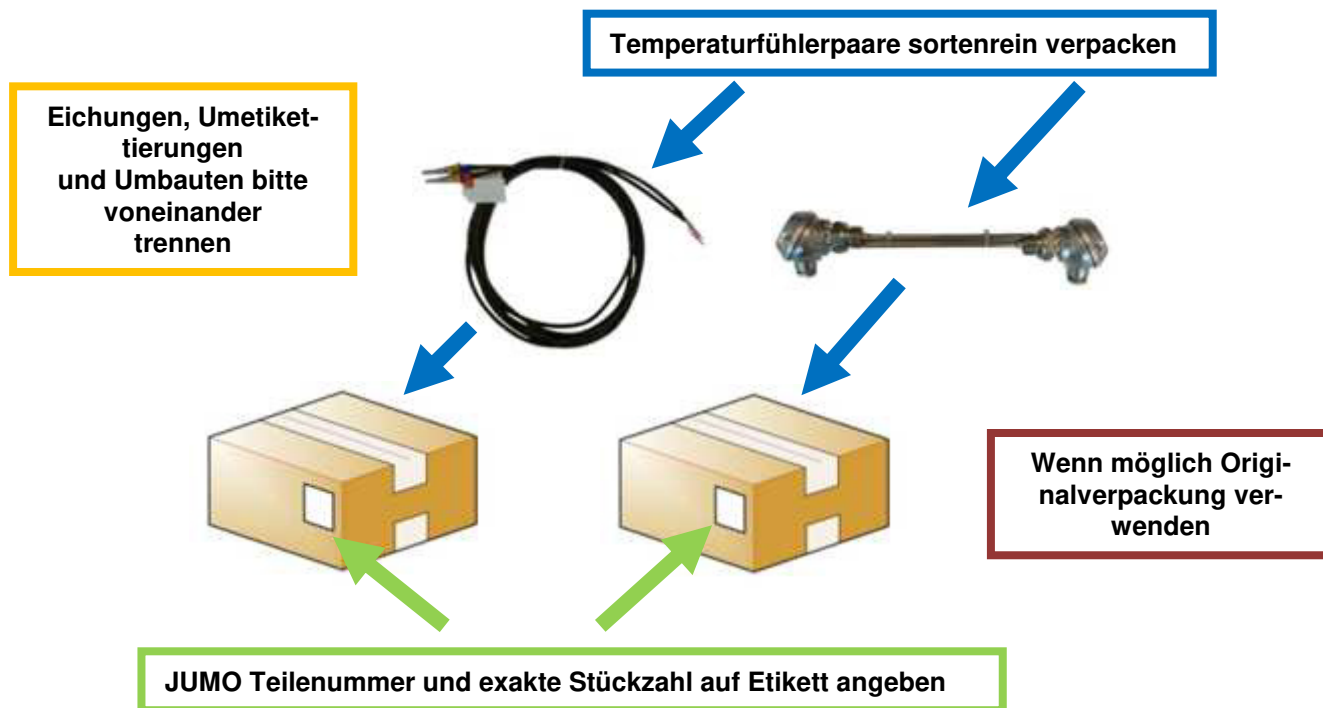


Verpackung / Versand	Temperaturfühlerpaare
<ul style="list-style-type: none"> • Wenn möglich Originalverpackung verwenden • Pro Karton nur 1 JUMO-Teilenummer ! • Fremdfabrikate sortenrein in eigene Kartons verpacken und nicht mit JUMO-Produkten mischen • JUMO-Teilenummer (wenn vorhanden) und exakte Anzahl der Temperaturfühlerpaare auf Karton (Etikett) und Lieferschein angeben, Sprache: Deutsch/Englisch 	<ul style="list-style-type: none"> • Bei Temperaturfühlerpaaren mit Einzelverpackungen –wenn möglich – Originalverpackung verwenden • Vor- und Rücklauffühler paarweise fixieren und sicher stellen, dass diese nicht während des Versands getrennt werden

Hinweise:

- Bitte „nicht paarbare“ (fehlerhafte) Temperaturfühlerpaarer aus den Eichungen der Vorjahre nicht erneut zusenden
- Temperaturfühlerpaare die nicht mehr geeicht werden konnten, werden zusammen in beschrifteten Tüten in Kartons verpackt
- Anfragen für einen möglichen Umbau von Temperaturfühlern / -paaren kann durch den Vertrieb geprüft und ein Angebot erstellt werden

Packaging instructions for the return of temperature probe pairs to JUMO

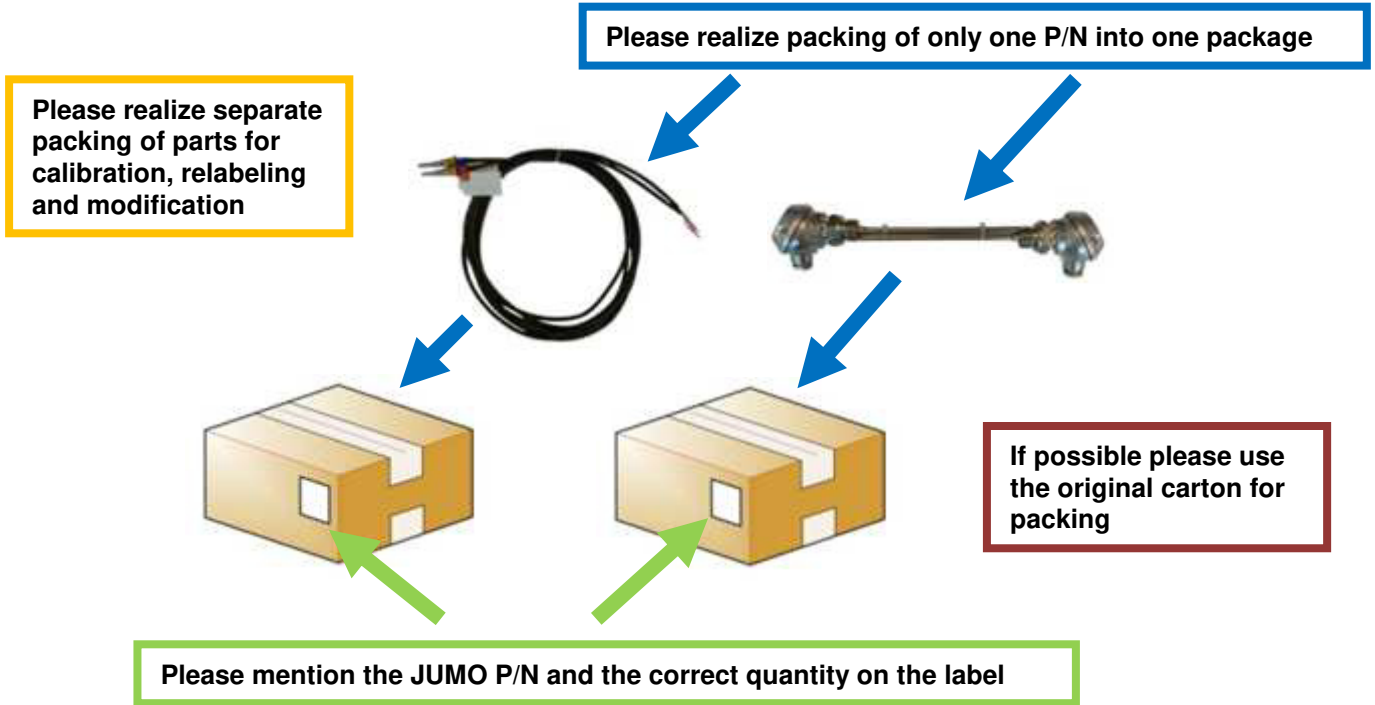

Packaging / dispatch	Temperature probe pairs
<ul style="list-style-type: none"> • If possible please use the original carton for packing • Please realize packing of only one P/N into one package! • Please realize packing of products from other companys separately • Please mention JUMO P/N (if available) and correct quantity of the temperature probe pairs on the carton (label) and the delivery note, language: German / English 	<ul style="list-style-type: none"> • For temperature probe pairs with single packing please use the original carton, if possible • Please arrange flow and return sensor in pairs and make sure that they are not separated during the transport

Remark:

- Please do not resend again (faulty) temperature probe pairs from the calibration of the previous year for which a pairing was not possible
- Temperature probe pairs for which a calibration was not possible are packed together in labeled bags
- Inquiries for a possible modification of the temperature probes / temperature probe pairs will be checked by the sales department and you will receive a corresponding quotation